


Amplivox 240, 260, 270 – Items required for calibration (items manufactured by G.R.A.S. & Digitron are shown as examples)



**Sound Level Meter
(G.R.A.S. HW1001)**

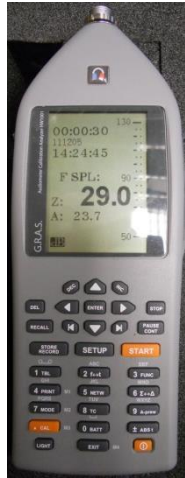

**Microphone calibrator
(G.R.A.S. 42AB)**



**Microphone
(G.R.A.S. 40AG)**



**Test stand (G.R.A.S. RA0052)
Artificial Ear (G.R.A.S. RA0039)**



**Microphone preamplifier/cable
(G.R.A.S. 26AM)**



**2cc coupler
(G.R.A.S. RA0038)**



**Artificial Mastoid
(Bruel & Kjaer 4930)**




**For 4930: Microdot cable
(G.R.A.S. AA0064)**



**For 4930: Microdot to
preamplifier adapter
(G.R.A.S. RA0125)**




**For 4930:
Thermometer
(Digitron 2000T)**



**For
Thermometer:
K type
thermocouple**

**Amplivox Model 270
Diagnostic Audiometer
Operating & Service Manual**
(Applies from serial number 7790 onwards)



Amplivox Ltd
6 Oasis Park
Eynsham
Oxfordshire
OX29 4TP
United Kingdom

Tel: +44 (0)1865 880846
Fax: +44 (0)1865 880426
sales@amplivox.ltd.uk
www.amplivox.ltd.uk

**Service manual
(Amplivox MANSERV)**