

Model 170

INSTRUCTION FOR USE



ABOUT THIS MANUAL

READ THIS OPERATING MANUAL BEFORE ATTEMPTING TO USE THE INSTRUMENT.

This manual is valid for the Model 170 (applies from firmware version 2N22 onwards – please refer to section 1.3).

This product is manufactured by:

Amplivox Ltd
3800 Parkside, Solihull Parkway,
Birmingham Business Park, Birmingham,
West Midlands,
B37 7YG
www.amplivox.com

For all enquiries please contact us under:

Amplivox Ltd
10393 West 70th Street
Eden Prairie
MN 55344
United States

Tel: 888 941 4208
Fax: 952 903 4100
info@amplivox.us

Amplivox Ltd
3800 Parkside, Solihull Parkway,
Birmingham Business Park, Birmingham,
West Midlands,
B37 7YG
United Kingdom
Tel: +44 (0)1865 880846

hello@amplivox.com



DGS Diagnostics A/S
Audiometer Alle 1
5500 Middelfart, Denmark

TABLE OF CONTENTS

ABOUT THIS MANUAL	1
TABLE OF CONTENTS	2
1. INTRODUCTION	4
1.1. THANK YOU	4
1.2. INTENDED APPLICATIONS	4
1.3. UNPACKING	4
1.4. FIRMWARE VERSION	4
1.5. STANDARD CONTENTS	4
1.6. OPTIONAL ACCESSORIES	5
1.7. OPTIONAL ACCESSORIES	5
2. IMPORTANT SAFETY INSTRUCTIONS	6
2.1. PRECAUTIONS	6
2.2. ELECTROMAGNETIC COMPATIBILITY (EMC) CONSIDERATIONS	6
2.3. POWER SUPPLY OPTIONS	6
2.4. AUDIOMETER CONNECTIONS	7
2.5. DATA TRANSFER TO A PRINTER	7
2.6. DATA TRANSFER TO A COMPUTER	8
3. USING THE AUDIOMETER	9
3.1. SWITCHING THE AUDIOMETER ON AND OFF	9
3.2. TESTING THE PATIENT RESPONSE SWITCH	9
3.3. AUDIOMETER DISPLAY	9
3.4. AUDIOMETER CONTROLS	9
3.4.1. Multifunction Keys	9
3.4.2. MENU	9
3.4.3. Description of Function of Other Keys	10
3.5. THRESHOLD RETENTION FUNCTION	11
3.5.1. Recording thresholds manually	11
3.5.2. Recording thresholds automatically	11
3.5.3. Reviewing retained thresholds	11
3.6. SAVING AUDIOGRAMS IN INTERNAL MEMORY	12
3.7. LOADING AUDIOGRAMS FROM INTERNAL MEMORY	12
3.8. PRINTING AUDIOGRAMS	12
3.9. DATA TRANSFER TO AUDIBASE OR AMPLISUITE	12
4. SUGGESTED SEQUENCE OF OPERATION AND TEST PROCEDURE	13
4.1. AUDIOMETRY PREPARATION AND AMBIENT CONDITIONS	13
4.2. TEST SYSTEM ARRANGEMENT	13
4.3. HEADSET	13
4.4. PATIENT INSTRUCTIONS	13
4.4.1. Pre-test	14
4.4.2. Familiarisation	14
4.4.3. Test	14
4.4.4. Post-test	14
4.4.5. Error messages	15
5. SPECIFICATION	16

5.1.	OUTPUT DATA	16
5.2.	MAXIMUM HEARING LEVELS PROVIDED AT EACH FREQUENCY	16
5.3.	PHYSICAL DATA	16
5.4.	EQUIPMENT CLASSIFICATION	17
6.	SYMBOLS	18
7.	TECHNICAL INFORMATION	19
8.	ROUTINE MAINTENANCE	20
8.1.	AUDIOMETER MAINTENANCE	20
8.2.	TRANSDUCER MAINTENANCE	20
8.3.	MAINS ADAPTER MAINTENANCE	20
9.	INSTRUMENT STORAGE AND TRANSPORTATION	21
10.	CALIBRATION AND REPAIR OF THE INSTRUMENT	21
11.	GUARANTEE	21
12.	ORDERING CONSUMABLES AND ACCESSORIES	22
13.	DISPOSAL INFORMATION	23
APPENDIX 1 - EMC GUIDANCE & MANUFACTURER'S DECLARATION		24
APPENDIX 2 - USE WITH NON-MEDICAL ELECTRICAL EQUIPMENT		28

1. INTRODUCTION

1.1. THANK YOU

Thank you for purchasing an Amplivox audiometer. The Amplivox Model 170 is an automatic screening audiometer that will give many years of reliable service if treated with care.

1.2. INTENDED APPLICATIONS

The Model 170 screening audiometer is designed for use by general practitioners, occupational health staff and child health professionals and is the ideal instrument for primary care groups, schools and industry. The audiometer may also be used for manual audiometry, but it is not intended for use to determine the full extent and scope of a patient's hearing deficiency.

Test results may be printed using the specified printer option or transferred to a PC running the Amplivox Audibase or AudiView applications.

1.3. UNPACKING

Open the shipping carton and carefully remove all the equipment. Check against the delivery note that all the accessories ordered have been included with your audiometer. If anything is missing, please contact Amplivox Customer Support (+44 1865 880846; sales@amplivox.ltd.uk). If you have purchased from a distributor you should contact them directly.

Please retain the shipping carton and packing materials as the audiometer will need calibrating on an annual basis and should be returned to Amplivox in its original shipping carton.

1.4. FIRMWARE VERSION

This operating manual is for firmware versions 4v47 onwards. To check the version of firmware on your audiometer press and hold the MENU button followed by the TALKOVER button.

1.5. STANDARD CONTENTS

Model 170 Audiometer	Audiometric headset
Carrying case	Patient response switch
Mains adapter	Audiogram cards
Operating manual & ampliSuite	Calibration certificate

1.6. OPTIONAL ACCESSORIES

Additional audiogram cards

Audibase software

USB Cable

Printer(s)

Printer cable(s)

Audiocups (noise reducing earphone enclosures)

1.7. OPTIONAL ACCESSORIES

Additional audiogram cards

Audibase software

USB Cable

Printer(s)

Printer cable(s)

Audiocups (noise reducing earphone enclosures)

2. IMPORTANT SAFETY INSTRUCTIONS



The Model 170 instrument must be used only by practitioners qualified to perform audiometric tests. It is intended for use as a screening tool.

2.1. PRECAUTIONS

READ THIS OPERATING MANUAL BEFORE ATTEMPTING TO USE THE INSTRUMENT

To comply with the standards IEC 60601-1 for safety and IEC 60601-1-2 for EMC the audiometer is designed to be used only with the medically-approved mains adapter supplied, which is specified as part of the equipment. **Do not use any other type of mains adapter with this instrument. Refer to Section 12 for the stock number of the adapter.**

The audiometer is for indoor use only and should be used only as described in this manual.

The transducers supplied with the audiometer are specifically calibrated with it; if these transducers are changed calibration will be required.

Do not immerse the unit in any fluids. See Section 8 of this manual for the proper cleaning procedure for the instrument and its accessories.

Do not use the instrument in an oxygen-rich environment or in the presence of a flammable anaesthetic mixture or other flammable agents.

Do not drop or otherwise impact this instrument. If the instrument is dropped or damaged, return it to the manufacturer for repair and/or calibration. Do not use the instrument if any damage is suspected.

The instrument must be stored and used within the specified temperature, pressure and humidity ranges (see Sections 7 and 9).

Do not attempt to open, modify or service the instrument. Return the instrument to the manufacturer or distributor for all repair and servicing requirements. Opening the instrument will void the warranty.

2.2. ELECTROMAGNETIC COMPATIBILITY (EMC) CONSIDERATIONS

Medical electrical equipment needs special precautions regarding EMC and needs to be installed and put into service according to the EMC information provided in Appendix 1. This provides guidance on the electromagnetic environment in which to operate the instrument.

Portable and mobile radio-frequency (RF) communications equipment can affect medical electrical equipment. The instrument should not be used adjacent to or stacked with other equipment; if this is necessary the instrument should be observed to verify normal operation.

2.3. POWER SUPPLY OPTIONS

All other connections must be made **before** connecting the output lead from the adapter into the POWER input socket on the back of the audiometer. Switch on the mains supply - the indicator on the adapter and the POWER indicator on the audiometer will both illuminate green, showing that the instrument is ready for use.

The output from mains adapter is fitted with electronic circuit protection. In case of overload the adapter will shut down and the indicator will be extinguished. When the fault is cleared the adapter will operate as normal.

The input to the mains adapter is protected with a non-replaceable fuse. If this fails the adapter will not operate.

The mains adapter is the mains disconnect device and therefore the audiometer should be positioned such that easy access to the mains adapter is possible.

If a replacement mains adapter is required, please contact Amplivox or your Amplivox distributor.

2.4. AUDIOMETER CONNECTIONS

All the relevant accessory terminals and connections are labelled to ensure correct identification and connection as follows:

Socket Label	Socket Type	Colour Code	Connected Part	Notes
RIGHT	6.3mm jack	Red	Air conduction headset *	
LEFT	6.3mm jack	Blue		
PRINTER	RJ12 socket (6-way)		Printer *	See 2.5
USB	USB Connector Type B		Computer (via USB port)	See 2.6
N/A	6 pin mini DIN		Reserved port; Amplivox diagnostic use only	See below
POWER	2.5mm power jack		Mains AC/DC Adapter *	
RESPONSE	6.3mm jack	Black	Patient Response Switch *	

The relevant part numbers are indicated in Section 12

Note regarding the 6-pin mini DIN connector:

This is a restricted socket for Amplivox use only. No user access is permitted.



For connected parts marked * only connect the accessories supplied with the instrument or supplied by Amplivox or an Amplivox distributor. These parts have been tested for use with the Model 170 Screening Audiometer for compliance with the standards IEC 60601-1 and IEC 60601-1-2. The use of accessories other than those specified may compromise compliance with these standards. For other sockets refer to Appendix 2.

2.5. DATA TRANSFER TO A PRINTER



Please refer to Appendix 2 for important information regarding the connection of non-medical electrical equipment to medical electrical equipment.

The audiometer can be upgraded with an option to allow connection to one of two designated portable thermal printers for printing audiometric test results (see Section 3.6). You must use the designated cable for each printer, which is supplied with this option.

Upon receipt of the printer it must be initially charged for a minimum of 15 hours prior to use.

2.6. DATA TRANSFER TO A COMPUTER



Please refer to Appendix 2 for important information regarding the connection of non-medical electrical equipment to medical electrical equipment.

The audiometer is supplied with software to allow connection to a computer for the transfer of test results (see Section 3.7). You must use the designated USB cable which is available from Amplivox (see Section 12).

3. USING THE AUDIOMETER

3.1. SWITCHING THE AUDIOMETER ON AND OFF

Press and briefly hold the switch marked  (located on the back panel). No warm-up time is required. The display will briefly show the model and the type of headphone currently in use. The display will then be similar to that shown in Section 3.3.

To switch off, press the switch marked  again, or press and hold the MENU key followed by the YES (RIGHT) key and then release both.

3.2. TESTING THE PATIENT RESPONSE SWITCH

Press the patient response switch and the light labelled RESPONSE (above and to the right of the display) will illuminate green.

3.3. AUDIOMETER DISPLAY

On start-up the display will show the following default setting:-

SIGNAL dBHL	FREQUENCY Hz
30dB	1kHz
< >	< >

This indicates that when the PRESENT key is pressed, a tone will be presented at 30dBHL at a frequency of 1kHz (1000Hz) to the designated ear. On start up the audiometer defaults to the left ear.

3.4. AUDIOMETER CONTROLS

3.4.1. MULTIFUNCTION KEYS

Several keys on the audiometer have different functions depending on the actual mode of operation. These are MENU (OFF), LEFT (NO), RIGHT (YES) and FREQUENCY   (MENU SELECT). The use of these keys is described below.

3.4.2. MENU

Press and hold MENU to access the following options. Use the MENU SELECT keys to step through the available options and then the NO, YES or SIGNAL   keys to select an action or modify a setting. Release of the MENU key then initiates the action or saves the modified setting and returns to the default display.

<u>Menu Option</u>	<u>Description</u>
Switch off?:	As described in Section 3.1
Clear test?:	Press YES and release MENU to clear the Threshold Retention Function results from the previous test
Save audiogram to (1):	Use the SIGNAL ↓↑ keys to select the required storage location and press the YES key to save the audiogram; then release MENU
Load audiogram no (1):	Use the SIGNAL ↓↑ keys to select the required storage location and press the YES key to load the audiogram; then release MENU
Contrast:	Adjust contrast using the SIGNAL ↓↑ keys; then release MENU
Print audiogram?:	Press YES and release MENU; then press YES to confirm the print operation or NO to cancel
Use 250Hz in auto?:	Press YES to include 250Hz in an automatic test or NO to exclude from the test
Use 1K5Hz in auto?:	Press YES to include 1.5kHz in an automatic test or NO to exclude from the test
Use 8KHz in auto?:	Press YES to include 8kHz in an automatic test or NO to exclude from the test
Use familiarization?:	Press YES to employ a familiarisation routine at the start of an automatic test sequence on either ear (see Section 4.5.2)
Store on 2 of 3?:	Press YES to activate automatic storage of the threshold level at which the patient makes 2 out of 3 responses in a manual test
Pulse?:	Press the YES key to output a pulse tone in mode
2 of 3 in auto?:	Press YES to activate automatic storage of the threshold level at which the patient makes 2 out of 3 responses in an automatic test (rather than the default 3 out of 5)
Default level:	Use the SIGNAL ↓↑ keys to adjust the default tone presentation level in manual mode
Select printer:	Use the MENU SELECT to select either the Able AP1300 or the Sanibel MPT-II printer

3.4.3. DESCRIPTION OF FUNCTION OF OTHER KEYS

PRINT	Press this key to print the current threshold levels; then press YES to confirm the print operation or NO to cancel
RESET	Press this key during an automatic test to cancel the test and return to the default display; any thresholds already found will be retained
+20dB	This enables tone levels to be presented with up to 20dB higher output in manual test mode; press the key and then use SIGNAL ↑ to access the extra 20dB in 5dB steps; an indicator above the key is used to show that the function is active
AUTO	This initiates an automatic test on the indicated ear (see Section 4.5)
RESULTS	Use this key at the conclusion of an automatic test to view the results (see Section 4.5.4)
TALK OVER	Hold this key to interrupt the test and route the operator's voice from the front panel microphone to the headset; the level is adjusted with the SIGNAL ↓↑ keys; if an

automatic test is in progress the current test frequency will be retested from the default level when the TALKOVER key is released

LEFT	Press once to select the left ear (the indicator above the key illuminates green); if the left ear is already selected press again to store the displayed signal value as a threshold (see Section 3.5.1)
RIGHT	Press once to select the right ear (the indicator above the key illuminates green); if the right ear is already selected press again to store the displayed signal value as a threshold (see Section 3.5.1)
SIGNAL	Press the $\downarrow\uparrow$ keys to decrease or increase the level of the tone presented in 5dB steps; to scroll through the range keep the key pressed
FREQUENCY	Press the $\leftarrow$ key to select a lower frequency and the $\rightarrow$ key to select a higher frequency
PRESENT	Press to present the displayed test signal to the patient. The “PRESENT” indicator above the display will be illuminated green during tone presentation.

3.5. THRESHOLD RETENTION FUNCTION

This function records the thresholds for both ears at each frequency tested. Thresholds may be recorded manually or automatically.

The operator can then review the results at the end of the test and record them on an audiogram card, print them with the optional printer (see Section 3.6), or transfer the results to a computer (see Section 3.7).

3.5.1. RECORDING THRESHOLDS MANUALLY

Once a threshold has been determined press the “selected” ear key once again. The threshold will be recorded and displayed as shown in the illustration in Section 3.5.3. **Note: this function will not operate if the “Store on 2 of 3” option has been enabled (see Section 3.5.2).**

3.5.2. RECORDING THRESHOLDS AUTOMATICALLY

If the “Store on 2 of 3” option has been enabled (see Section 3.4.2) then a threshold will be recorded automatically by the audiometer if the patient makes a response to two out of three manual tone presentations at the same level and frequency. Thresholds determined using the “Store on 2 of 3” option are displayed within square brackets.

3.5.3. REVIEWING RETAINED THRESHOLDS

To review the retained thresholds, select the required frequency using the FREQUENCY $\leftarrow \rightarrow$ keys. The recorded values for the left and right ears are shown on the lower line of the display as illustrated below.

SIGNAL dBHL

FREQUENCY Hz

30dB	4kHz
20	10

THRESHOLDS

This display shows thresholds at 4kHz

Left ear 20dBHL

Right ear 10dBHL

To clear the Threshold Retention memory, use the Clear Test menu option described in Section 3.4.2.

3.6. SAVING AUDIOGRAMS IN INTERNAL MEMORY

The user may save up to 12 audiograms, referenced by number, in the internal memory of the audiometer. To save the current set of audiogram thresholds (these are the “retained” values described in Section 3.5) press and hold the MENU key, and then press MENU SELECT repeatedly until “Save Audiogram to 1” appears on screen. Use the SIGNAL ↓↑ keys to select a location numbered 1-12, and then press the YES key. Release the MENU key once confirmation appears on the display.

Note that the Save process will overwrite any records that exist in the selected memory location.

3.7. LOADING AUDIOGRAMS FROM INTERNAL MEMORY

Press and hold the MENU key, and then press MENU SELECT repeatedly until “Load Audiogram No 1” appears on screen. Use the SIGNAL ↓↑ keys to select a location numbered 1-12, and then press the YES key. Release the MENU key once confirmation appears on the display.

3.8. PRINTING AUDIOGRAMS

Two designated thermal printers (the Able AP1300 or the Sanibel MPT-II) are available as options for use with the Model 170 audiometer. The correct printer must be selected (use the MENU options described in Section 3.4.2 to make this selection).

- Connect the PRINTER socket on the audiometer (6-way RJ12) to the printer with the supplied cable (refer to Section 2.5 of this operating manual for printer set-up). **Note that the printer cables for the Able printer (A108) and Sanibel (A102) are not compatible.**
- Ensure that the printer is fully charged, switched on, loaded with paper and ready to print.
- Press the PRINT key and on the prompt “Is printer ready?” press the YES key. The audiogram will then print. To cancel press NO.

3.9. DATA TRANSFER TO AUDIBASE OR AMPLISUITE

Test results stored within the audiometer may be transferred to the Amplivox Audibase database which is available as an option and must be installed on to a computer (see Section 12 for the part number). Alternatively, Amplivox ampliSuite allows data to be transferred to a computer and subsequently viewed, annotated & printed. This software is supplied on a USB which includes this operating manual.

Refer to the installation & operating instructions provided with Audibase or ampliSuite for further details.

4. SUGGESTED SEQUENCE OF OPERATION AND TEST PROCEDURE

The following applies to air conduction measurements. Refer also to ISO 8253 for guidance.


4.1. AUDIOMETRY PREPARATION AND AMBIENT CONDITIONS

Refer to the appropriate audiometric standards and other relevant publications for guidance on audiometric testing.

Audiometric testing should always be performed in quiet conditions (e.g. a quiet room or an acoustic booth). The optional Audiocups can provide an additional level of isolation from ambient noise. For further explanation on permissible ambient noise levels, please refer to the standard ISO6189.

4.2. TEST SYSTEM ARRANGEMENT

The schematic diagram below shows a typical example of the use of audiometric test equipment. The audiometer is located on the desk of a seated operator as shown.

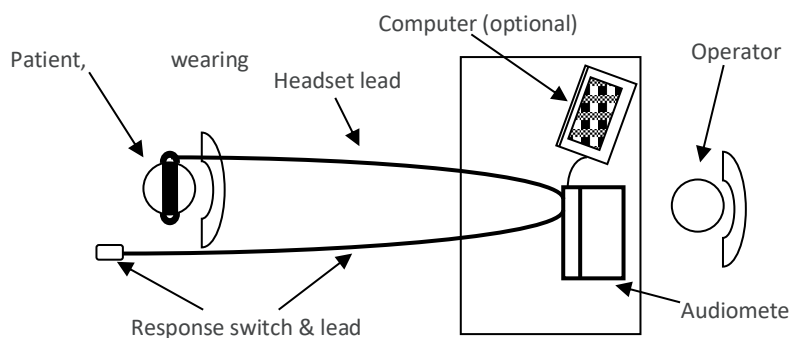

The patient is seated in front of the desk facing away from the operator. The patient wears a headset (see Section 4.3) and responds to test stimuli by use of a hand-held switch which is also connected to the instrument.

4.3. HEADSET

The headset must be fitted by a qualified person to ensure a proper seal and a comfortable fit. The leads from the headset are connected to the instrument and the headset is then fitted to the patient.

4.4. PATIENT INSTRUCTIONS

The patient should be given the following instructions using the TALKOVER function:

- "As soon as you hear the tone, press the response switch. When you no longer hear the tone release the response switch"

4.4.1. PRE-TEST

- (1) Switch the audiometer on
- (2) Perform a listening check
- (3) Decide whether to use the manual or automatic Threshold Retention Function and/or an audiogram card to record the thresholds
- (4) If the automatic Threshold Retention Function is required ensure that the Store on 2 of 3 option is enabled (see Section 3.5.2) and that a patient response switch is in use
- (5) Prepare the test environment & patient (see Sections 4.1 to 4.4)
- (6) If the patient response switch is not being used give instructions to the patient to acknowledge any tone presented by raising or lowering the finger
- (7) Select the better hearing ear (according to the patient) by pressing either the LEFT or RIGHT key and start the familiarisation session.

4.4.2. FAMILIARISATION

- (1) Present the tone 30dB at 1kHz for between 1 and 2 seconds. If there is no response at 30dB, increase the attenuation level in 10dB steps until the patient responds
- (2) When the patient responds, wait for 1 to 2 seconds and present the tone again at the same level; however, if the patient does respond at 30dB, reduce the signal level in 10dB steps, repeating the presentation until there is no response, then increase the signal level in 5dB steps until the patient responds; wait 1 to 2 seconds and present the tone again at the same level
- (3) If the responses are consistent with the pattern of tone presentation proceed to Section 4.7 and start measuring the patient's hearing thresholds; if not, repeat the familiarisation process

4.4.3. TEST

- (1) Present the first test tone at 30dB at 1kHz
- (2) If the patient responds, reduce the signal level in 10dB steps repeating the presentation until there is no response; then increase the signal level in 5dB steps until the patient responds
- (3) If the patient does not respond, increase the signal level in 5dB steps until there is a response and then continue with step 4.
- (4) Repeat the test by reducing the signal level in 10dB steps until the patient no longer responds. Then increase the signal level in 5dB steps until they do respond and note this level.
- (5) Repeat step 4 until the patient responds three out of a maximum of five times at the same signal level. This indicates the patient's hearing threshold level for that frequency. Either mark the threshold on an audiogram card or press the appropriate ear key once to activate the Threshold Retention Function and save the threshold level on screen.
- (6) Proceed to the next test frequency. It is common practice to test the frequencies in the following order: 1k, 2k, 3k, 4k, 6k, 8k and 500 Hz.
- (7) Repeat steps 1 to 6 for the other ear.

4.4.4. POST-TEST

- (1) Use the Threshold Retention Function to review the results (See 3.5)
- (2) If required do one or more of the following:
 - Record the results on an audiogram card, or
 - Print the results (Section 3.6), or
 - Transfer the results to a computer (Section 3.7)

Refer to Section 3.4.2 to clear the thresholds at the end of a test and, if required, switch off the audiometer.

4.4.5. ERROR MESSAGES

Four error messages are possible while an automatic test is running. Depending on circumstances it may be necessary to provide further instruction to the patient and/or perform manual familiarisation (see Section 4.4.2).

No response!

This occurs when the patient has made no response and the tone level has reached the maximum value. An option to repeat the test at that frequency is presented. Press YES to repeat or NO to skip to the next frequency. If the frequency is skipped the message “Test finished incomplete” will be displayed at the conclusion of the test.

Response always!

This indicates that the patient has not released the response switch and the tone level has reached the minimum value. An option to repeat the test at that frequency is presented. Press YES to repeat or NO to skip to the next frequency. If the frequency is skipped the message “Test finished incomplete” will be displayed at the conclusion of the test.

1kHz match exceeded!

This occurs when the threshold level found at the 1kHz re-test differs by more than 10dB from that found for the 1st test (see Section 4.5.3). An option to repeat the re-test is presented. Press YES to repeat or NO to accept the threshold level found at the re-test.

Test finished incomplete

This occurs if the audiometer was unable to record a threshold at one or more frequencies (e.g. if no response was made and the retry option was not chosen). The operator then has the option to use manual audiometry to obtain any missing thresholds.

5. SPECIFICATION

5.1. OUTPUT DATA

Outputs:	Left and Right earphone
Frequency range:	125Hz to 8kHz
Frequency accuracy:	<1%
Distortion:	<2%
Output level range:	-10dBHL min; see Section 5.2 for maximum
Output level accuracy:	Within 3dB
Output level step size:	5dB
Output transducer:	DD45 earphones (supplied), IP30 insert earphones (option)
Tone present:	Single, warble or pulsed
Communication:	Integral talk over facility
USB interface:	Transfer of test results to a computer

5.2. MAXIMUM HEARING LEVELS PROVIDED AT EACH FREQUENCY

Frequency, Hz	Air conduction, dBHL	Frequency, Hz	Air conduction, dBHL
125	70	2000	100
250	80	3000	100
500	90	4000	100
750	100	6000	100
1000	100	8000	80
1500	100		

5.3. PHYSICAL DATA

Display:	2 lines of 24 characters
Mains Power:	100-240Vac; 50-60Hz; 0.5A
Input Rating:	5Vdc; 1.2 A
Dimensions:	270mm long x 165mm deep x 60mm high
Weight:	0.75kg (approx)
Safety:	IEC 60601-1 (plus UL, CSA & EN deviations)

EMC: IEC 60601-1-2
CE mark: To the EU Medical Device Regulation

5.4. EQUIPMENT CLASSIFICATION

Type of protection against electric shock	Powered via SELV ClassII mains adapter
Degree of protection against electric shock	Type B applied part
Degree of protection against ingress of water	Not protected
Mode of operation	Continuous operation
Equipment mobility	Portable

The Model 170 Audiometer is classified as a Class IIa device under Annex II of the EU Medical Devices Regulation. It is intended for use as a screening audiometer instrument.

6. SYMBOLS

The following symbols appear on the audiometer or mains adapter:



Definition: Identifies the control by means of which the instrument is switched on from (or returned to) a standby condition.



Definition: Medical device



Definition: Refer to instruction manual (mandatory).




Definition: Type B applied part – an applied part providing protection against electric shock, particularly regarding allowable patient leakage current and patient auxiliary current.

The applied parts are the left & right earphones, patient response switch and the associated cables.



Definition: The output from the mains AC adapter is Direct Current.



Definition: Class II equipment – equipment in which protection against electric shock does not rely on basic insulation only, but in which additional safety precautions such as double insulation or reinforced insulation are provided, there being no provision for protective earthing or reliance upon installation conditions.

7. TECHNICAL INFORMATION

Audiometer

Audiometer type: Type 4 (IEC 60645-1:2001)
 Type 4 (ANSI S3.6:2004)

Transducers

Types and reference levels: DD45: ISO 389-1, Table 2
 IP30: ISO 389-2, Table 1

Static headband force: Headphones: 4.5N

Sound attenuation characteristics: ISO8253-1, Table 3

Earphone Sound Attenuation Characteristics

Frequency, Hz	125	250	500	1000	2000	4000	8000
Attenuation, dB	2	5	7	15	25	31	23

Environmental

Operating temperature: +15°C to +35°C

Operating humidity: 30% to 90% (non-condensing)

Atmospheric pressure: 700 hPa to 1060 hPa

Input / Output

Power input: 2.5mm barrel-type socket.

Patient response input: 6.3mm Jack socket

Left & Right outputs: 6.3mm Jack socket

USB: Type B socket

Printer: RJ12 socket (6-way)

Maximum voltage at any output: 12V peak

8. ROUTINE MAINTENANCE

8.1. AUDIOMETER MAINTENANCE

The Model 170 audiometer is a precision instrument. Handle it carefully in order to ensure its continued accuracy and service. When cleaning the instrument, first disconnect it from the mains supply. Use a soft cloth and mild detergent to clean the instrument panel when required. Refer to ISO 8253-1 for additional guidance.

8.2. TRANSDUCER MAINTENANCE

Before use check the transducer cables and connectors for signs of wear and/or damage. If you find any, please replace the item immediately by contacting Amplivox or your Amplivox distributor, requesting the relevant part number (see Section 12).

Handle the audiometric headset and other accessories with care. For parts that are in direct contact with the patient it is recommended that replacement parts are used or the parts are subjected to a standard disinfecting procedure between patients.

This includes physically cleaning and use of a recognised disinfectant. The specific manufacturer's instructions should be followed for use of this disinfecting agent to provide an appropriate level of cleanliness.

Clean the ear cushions (including those on the Audiocups, if used) with a recognised disinfectant, e.g. a "Mediswab".



During the cleaning process do not allow moisture to enter the earphone.

8.3. MAINS ADAPTER MAINTENANCE

Before use check the mains AC adapter for signs of wear and/or damage. If you find any replace the adapter immediately by contacting Amplivox or your Amplivox distributor. Refer to Section 12 for approved part numbers.



DO NOT USE ANY OTHER TYPE OF MAINS ADAPTER WITH THIS INSTRUMENT. See Section 2.3.

9. INSTRUMENT STORAGE AND TRANSPORTATION

This instrument can be stored or transported within the following environmental parameters:

Temperature:	-20°C to +70°C
Humidity:	10% to 90% (non-condensing)
Atmospheric Pressure:	500 hPa to 1060 hPa

10. CALIBRATION AND REPAIR OF THE INSTRUMENT

Amplivox recommends that this audiometer should be calibrated on an annual basis. Please contact Amplivox or the designated distributor for details of calibration services. Refer to ISO 8253-1 for additional guidance.



The instrument should be returned to the manufacturer for service & repair. There are no user-serviceable parts within it.

When packing the instrument for shipping, please use the original shipping carton and packing materials. Please also ensure that the headset leads are not wrapped around the headband of the headset.

11. GUARANTEE

All Amplivox instruments are guaranteed against faulty materials and manufacture. The instrument will be repaired free of charge for a period of three years from the date of despatch if returned, carriage paid, to the Amplivox service department. Return carriage is free of charge for customers in the UK and chargeable for overseas customers.

Important Note:

The following exceptions apply:

Earphones may go out of calibration due to rough handling or impact (dropping). The life of the leads is also dependent upon conditions of use. These parts are only guaranteed against faulty materials or manufacture.

12. ORDERING CONSUMABLES AND ACCESSORIES

To order consumables, additional accessories and to replace detachable parts that have been damaged, please contact Amplivox for current prices and delivery charges. The items available are listed below:

Stock No.		Description
A022	8010855	Audiocups (noise reducing earphone enclosures)
AC1042	8010835	Audiocup ear cushion
AC1047	8507920	Audiocup headband
AC1048	8010834	Audiocup headband cover
A023	8010882	Headband (standard headphone)
A026	8010857	Earphone cushion
A032	8010876	Earphones DD45 *
A030	8010822	Headset lead
B128	8532675	Carrying case
	8512734	Approved mains adapter (UE12LCP)
A085	8011155	Patient response switch
A051	8013007	Audiogram cards (pack of 50)
PT02	8535338	Printer Sanibel MPT-II
A102	8004419	Printer cable for audiometer to Sanibel MPT-II
C0104	8029305	Thermal Printer paper for Sanibel MPT-II
F07	8011241	USB Cable, 2.0m
AUD06	8511500	Amplivox Audibase 5.5 (including USB cable)



Accessories marked * require calibration with the specific audiometer to be used. Do not attempt to use these accessories until the audiometer has been calibrated to match their characteristics.

Shipping documentation will reference the stock number quoted above, and images of the parts alongside the relevant stock number are available on the Amplivox website (www.amplivox.ltd.uk). The required fitting instructions are supplied with each part.

13. DISPOSAL INFORMATION



Amplivox Limited is fully compliant with the WEEE (Waste Electrical and Electronic Equipment) Regulations. Our PRN (Producer Registration Number) is WEE/GA0170XU and we are registered with the approved WEEE Compliance Scheme, B2B Compliance, approval number WEE/MP3338PT/SCH.

The main purpose of the WEEE Regulations is to encourage the segregation of waste electrical items from the general waste stream and into reuse, recovery and recycling routes.

For any waste electrical units purchased from Amplivox that either:

- bear the crossed out wheeled bin symbol with black bar underneath
 - or, have been replaced with new Amplivox products on a like-for-like basis
- please contact our WEEE Compliance Scheme using the details below. B2B Compliance will be able to provide further information on how to recycle your waste electrical units and answer any queries you may have.

B2B Compliance

Tel: +44 (0) 1691 676 124 (Option 2)

Email: operations@b2bcompliance.org.uk

APPENDIX 1 - EMC GUIDANCE & MANUFACTURER'S DECLARATION

Guidance and manufacturer's declaration – electromagnetic emissions		
The Model 170 Audiometer is intended for use in the electromagnetic environment specified below. The customer or user of Model 170 Audiometer should assure that it is used in such an environment.		
Emissions test	Compliance	Electromagnetic environment – guidance
RF emissions CISPR 11	Group 1	The Model 170 Audiometer uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause interference in nearby electronic equipment. The Model 170 Audiometer is suitable for use in all establishments, including domestic establishments and those directly connected to the public low-voltage power supply network that supplies buildings used for domestic purposes.
RF emissions CISPR 11	Class B	
Harmonic emissions IEC 61000-3-2	Class A	
Voltage fluctuations/flicker emissions IEC 61000-3-3	Complies	

Guidance and manufacturer's declaration – electromagnetic immunity (1)			
The Model 170 Audiometer is intended for use in the electromagnetic environment specified below. The customer or user of the Model 170 Audiometer should assure that it is used in such an environment.			
Immunity test	IEC 60601 test level	Compliance level	Electromagnetic environment – guidance
Electrostatic Discharge (ESD) IEC 61000-4-2	±8 kV contact ±15 kV air	±8 kV contact ±15 kV air	Floors should be wood, concrete or ceramic tile. If floors are covered with synthetic material, the relative humidity should be at least 30%
Electrical fast transient/burst IEC 61000-4-4	±2 kV for power supply lines ±1 kV for input/output lines	±2 kV for power supply lines ±1 kV for input/output lines	Mains power quality should be that of a typical commercial or hospital environment
Surge IEC 61000-4-5	±1 kV differential mode ±2 kV common mode	±1 kV differential mode ±2 kV common mode	Mains power quality should be that of a typical commercial or hospital environment

Immunity test	IEC 60601 test level	Compliance level	Electromagnetic environment – guidance
Voltage dips, short interruptions and voltage variations on power supply input lines (100V/60Hz & 240V/50Hz) IEC 61000-4-2	0% UT (100% dip in UT) for 0.5 cycle 0% UT (100% dip in UT) for 1 cycle 40% U_T (60% dip in U_T) for 5 cycles 70% UT (30% dip in UT) for 500ms 0% UT (100% dip in UT) for 5 sec	0% UT 100% dip in UT) for 0.5 cycle 0% UT (100% dip in UT) for 1 cycle 40% U_T (60% dip in U_T) for 5 cycles 70% UT (30% dip in UT) for 500ms 0% UT (100% dip in UT) for 5 sec	Mains power quality should be that of a typical commercial or hospital environment. If the user of the Model 170 Audiometer requires continued operation during power mains interruptions, it is recommended that the Model 170 Audiometer be powered from an uninterruptible power supply or a battery
Power frequency (50/60 Hz) magnetic field IEC 61000-4-8	30 A/m	30 A/m	Power frequency magnetic fields should be at levels characteristic of a typical location in a typical commercial or hospital environment.
NOTE U_T is the a.c. mains voltage prior to the application of the test level			

Guidance and manufacturer's declaration – electromagnetic immunity (2)			
The Model 170 Audiometer is intended for use in the electromagnetic environment specified below. The customer or user of the Model 170 Audiometer should assure that it is used in such an environment.			
Immunity test	IEC 60601 test level	Compliance level	Electromagnetic environment – guidance
Conducted RF IEC 61000-4-6	10 Vrms 150kHz to 80MHz	10 Vrms 150kHz to 80MHz	Portable and mobile RF communications equipment should be used no closer to any part of the Model 170 Audiometer, including cables, than the recommended separation distance calculated from the equation applicable to the frequency of the transmitter. Recommended separation distance $d = 1.2\sqrt{P}$ $d = 1.2\sqrt{P}$ 80MHz to 800MHz $d = 2.3\sqrt{P}$ 800MHz to 2.5GHz where P is the maximum output power rating of the transmitter in Watts (W) according to the transmitter manufacturer and d is the recommended separation distance in metres (m). Field strengths from fixed RF transmitters, as determined by an electromagnetic site survey,^a should be less than the compliance level in each frequency range.^b Interference may occur in the vicinity of equipment marked with the following symbol:
Radiated RF IEC 61000-4-3	10 V/m 80MHz to 2.7GHz	10 V/m 80MHz to 2.7GHz	

Guidance and manufacturer's declaration – electromagnetic immunity (2)			
NOTE 1 At 80MHz and 800MHz, the higher frequency range applies.			
NOTE 2 These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.			
a	Field strengths from fixed transmitters, such as base stations for radio (cellular/cordless) telephones and land mobile radios, amateur radio, AM and FM radio broadcast and TV broadcast cannot be predicted theoretically with accuracy. To assess the electromagnetic environment due to fixed RF transmitters, an electromagnetic site survey should be considered. If the measured field strength in the location in which the Model 170 Audiometer is used exceeds the applicable RF compliance level above, the Model 170 Audiometer should be observed to verify normal operation. If abnormal performance is observed, additional measures may be necessary, such as re-orienting or relocating the Model 170 Audiometer.		
b	Over the frequency range 150 kHz to 80 MHz, field strengths should be less than 3 V/m.		
Recommended separation distances between portable and mobile RF communications equipment and the Model 170 Audiometer			
The Model 170 Audiometer is intended for use in an electromagnetic environment in which radiated RF disturbances are controlled. The customer or the user of the Model 170 Audiometer can help prevent electromagnetic interference by maintaining a minimum distance between portable and mobile RF communications equipment (transmitters) and the Model 170 Audiometer as recommended below, according to the maximum output power of the communications equipment.			
Rated maximum output power of transmitter W	Separation distance according to frequency of transmitter		
	m		
	150 kHz to 80 MHz	80 MHz to 800 MHz	800 MHz to 2.5 GHz
	d = 1.2√P	d = 1.2√P	d = 2.3√P
0.01	0.12	0.12	0.23
0.1	0.38	0.38	0.73
1	1.2	1.2	2.3
10	3.8	3.8	7.3
100	12	12	23
For transmitters rated at a maximum output power not listed above, the recommended separation distance d in metres (m) can be estimated using the equation applicable to the frequency of the transmitter, where P is the maximum output power rating of the transmitter in Watts (W) according to the transmitter manufacturer.			
NOTE 1 At 80MHz and 800MHz, the separation distance for the higher frequency range applies.			
NOTE 2 These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.			
NOTE 3 WARNING: Portable RF communications equipment (including peripherals such as antenna cables and external antennas) should be used no closer than 30cm (12 inches) to any part of the Model 170 audiometer including cables specified by the manufacturer. Otherwise degradation of the performance of this equipment could result.			

APPENDIX 2 - USE WITH NON-MEDICAL ELECTRICAL EQUIPMENT

Any person who connects external equipment to signal input, signal output or other connectors has created a medical electrical system and is therefore responsible for the system complying with the requirements of clause 16 of IEC 60601-1:2005 (*General requirements for basic safety and essential performance*).

If connections are made to standard equipment such as printers and computers, special precautions must be taken in order to maintain medical safety. The following notes are provided for guidance in making such connections to ensure that the general requirements of clause 16 of IEC 60601-1:2005 are met.

The following signal inputs and outputs on the Model 170 audiometer are electrically isolated to the requirements of IEC 60601-1 in order to reduce any potential hazard associated with the use of mains-powered equipment connected to these inputs and outputs:

Socket Label	Socket Type	Typical Connection
PRINTER	RJ12 socket (6-way)	Printer
USB	USB Connector Type B	Computer

External equipment intended for connection to signal input, signal output or other connectors, shall comply with the relevant IEC or international standards (e.g. IEC 60950, CISPR 22 & CISPR 24 for IT equipment, and the IEC 60601 series for medical electrical equipment).

Equipment not complying with IEC 60601 shall be kept outside the patient environment, as defined in IEC 60601-1:2005 (at least 1.5m from the patient).

The operator must not touch the connected equipment and the patient at the same time as this would result in an unacceptable hazard.

Refer to Diagrams 1 to 3 below for typical configurations of connected peripheral equipment. Refer to Amplivox Limited at the address given on the front of this user manual if advice is required regarding the use of peripheral equipment.

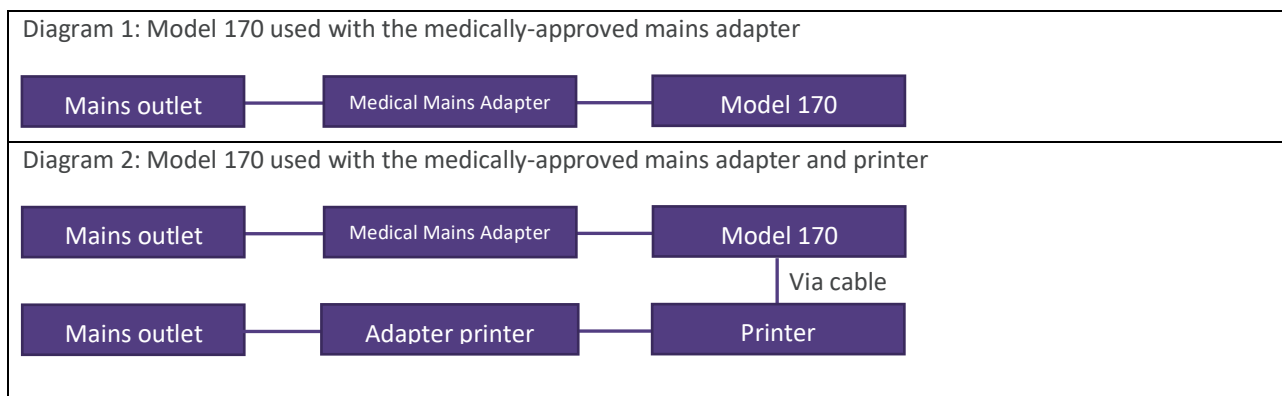


Diagram 3: Model 170 used with the medically-approved mains adapter and PC

